

Safety and Effectiveness of Smooth Incision Lenticular Keratomileusis (SILK™) Using the ELITA™ Femtosecond Laser System for Correction of Myopic and Astigmatic Refractive Errors [Corrigendum]

Sachdev MS, Shetty R, Khamar P, et al. *Clin Ophthalmol.* 2023;17:3761-3773.

The authors have advised that there are errors in Figure 3A and B on page 3767. The X and Y axes and all other numbers should be shown as negative (–) rather than positive (+). The correct Figure 3 is as follows.

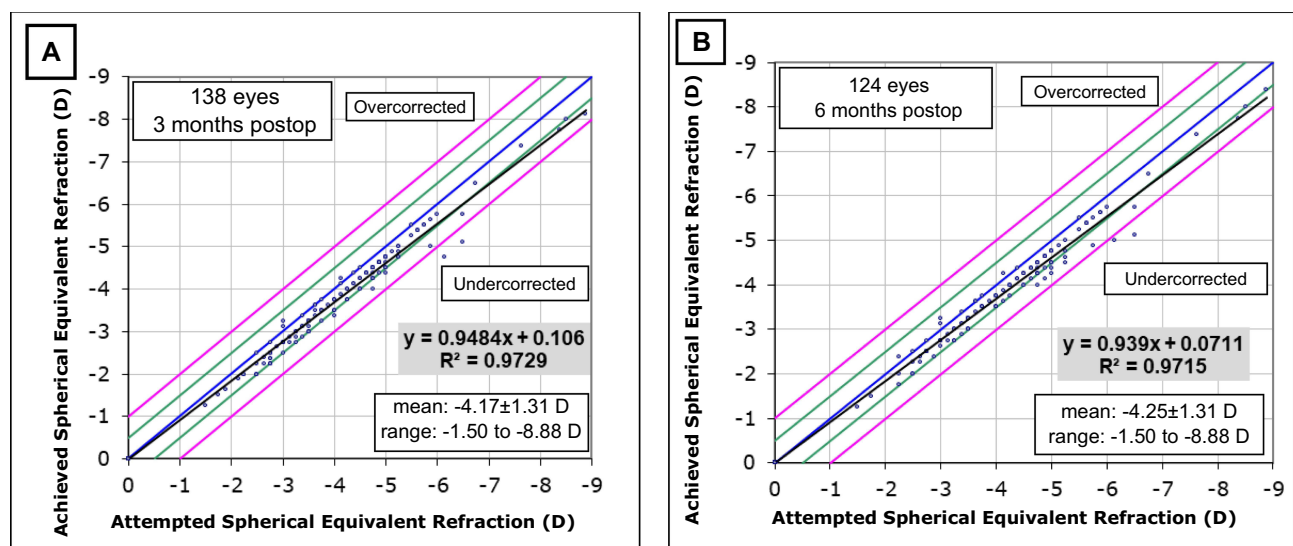


Figure 3 Attempted versus achieved spherical equivalent refraction at (A) 3 and (B) 6 months. The blue line indicates a perfect result, and the green and pink lines depict over- and under-correction of 0.50 D and 1.00 D, respectively.

The authors apologize for these errors.